ASSESSMENT OF DIFFERENTIAL PRESSURES ACROSS STERILIZING FILTER MEMBRANES WITH VARIOUS TEST SOLUTIONS

Zachary Bendiks, Ph.D., Leesa McBurnie


Abstract

FDA recommends monitoring differential pressure across filter membranes during sterile filtration process validation. However, few resources are available to help pharmaceutical manufacturers anticipate expected differential pressures during sterilizing filtration of different solutions. To address this gap, Meissner evaluated differential pressures across different filtration membranes using various test solutions at increasing pump speeds. Specifically, we investigated differential pressures across sterilizing-grade PVDF, PES, and PTFE membrane discs, either in series or with downstream 0.4 µm PES analysis discs commonly used in bacterial retention testing. The test solutions employed for this study include saline, grapeseed oil, FBS, and DMEM cell culture media with 10% FBS. These solutions were chosen based on their differing physicochemical properties and their relevance to the pharmaceutical industry. This work will serve as a reference for pharmaceutical manufacturers and help them anticipate differential pressures across sterilizing filter membranes at different pump speeds based on the physicochemical properties of their drug products.

Material Methods

The test solutions were 0.85% saline, 100% grapeseed oil, fetal bovine serum (FBS), or Dulbecco's Modified Eagle Medium (DMEM) with 10% FBS. Prior to testing, the grapeseed oil was pre-filtered with a 0.2 µm polyethersulfone (PES) capsule and warmed to 30 °C. All other solutions were tested at room temperature. The DMEM + 10% FBS was pre-filtered with a 0.2 µm polyvinylidyne fluoride (PVDF) disc.


Approximately 1 L of test solution was recirculated through two 47 mm discs installed in disc holders using a peristaltic pump at increasing pump speeds. The 47 mm disc membranes were 0.1 or 0.2 µm polyethersulfone (PES), polyvinylidyne fluoride (PVDF), or polytetrafluoroethylene (PTFE), either in series to simulate redundant filtration or with downstream 0.4 µm PES discs to simulate bacterial retention testing. Pressures upstream of each filter disc were measured using calibrated Anderson pressure gauges installed on single-use gauge tees. Differential pressure was determined by calculating the difference between the upstream and downstream pressure gauges. All values below 2 psi were recorded as 0 psi.

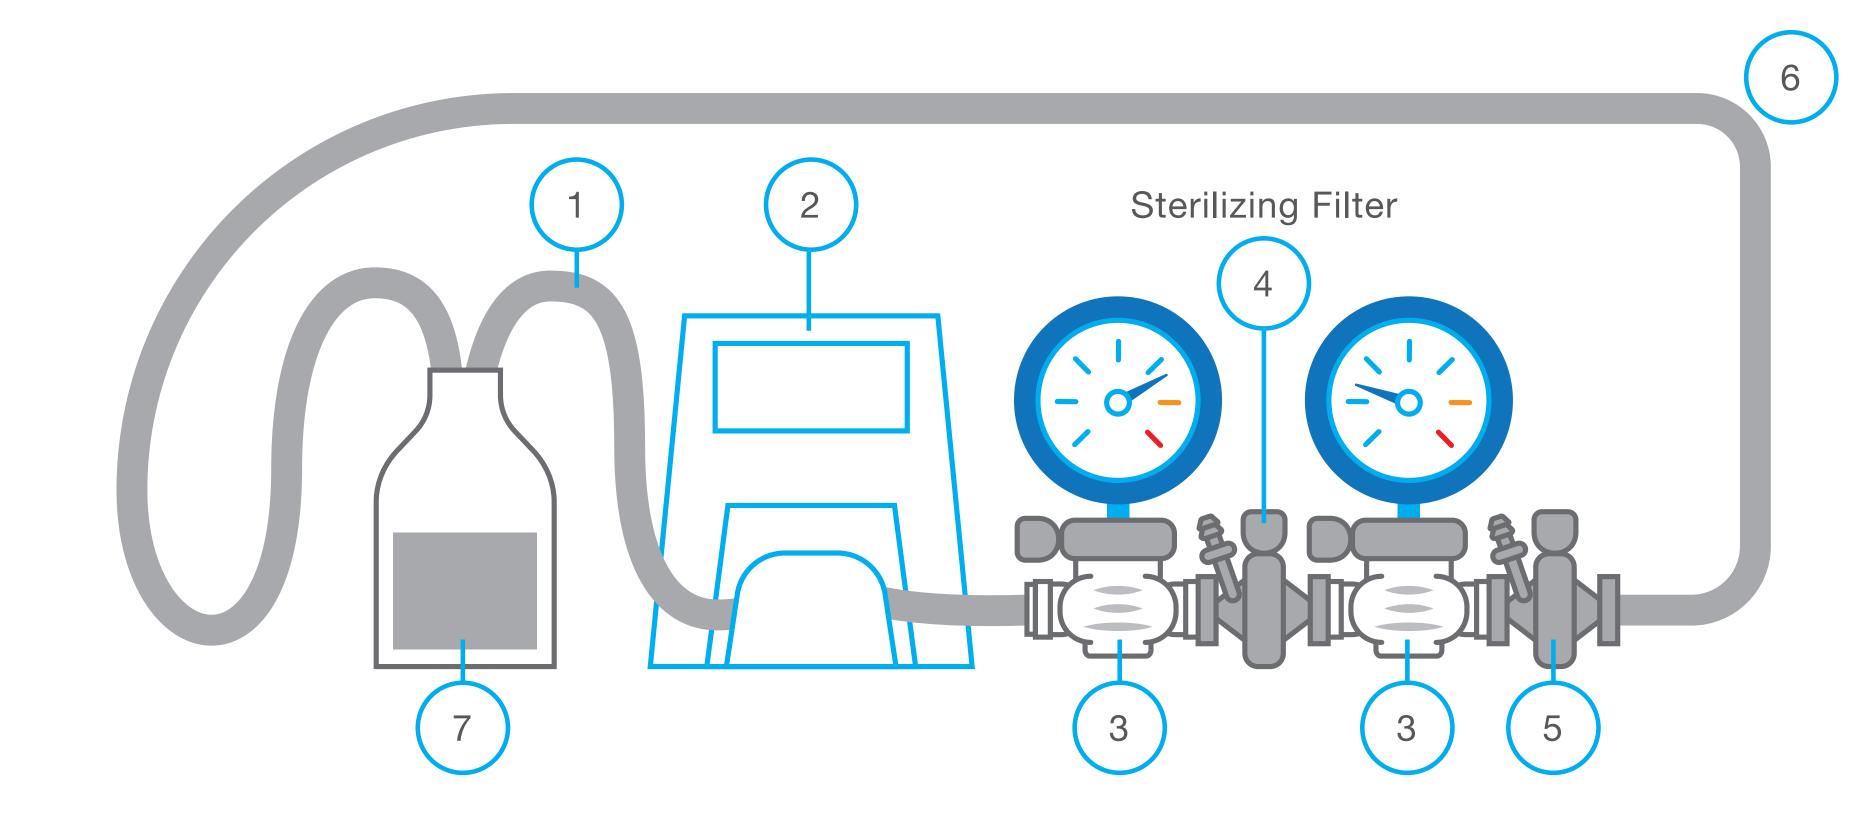



- . Upstream TPE pump tubing
- 2. Peristaltic pump
- 3. Pressure gauge, Single-use Gauge Tee (SGT), large clamp, 2x small gaskets, and clamps
- 4. Sterilizing filter in holder
- 5. Redundant sterilizing filter or 0.4 µm PES analysis filter in holder
- 6. Downstream silicone tubing with fitting, small gasket, and clamp
- 7. 1 L media bottle containing test solutions


Results




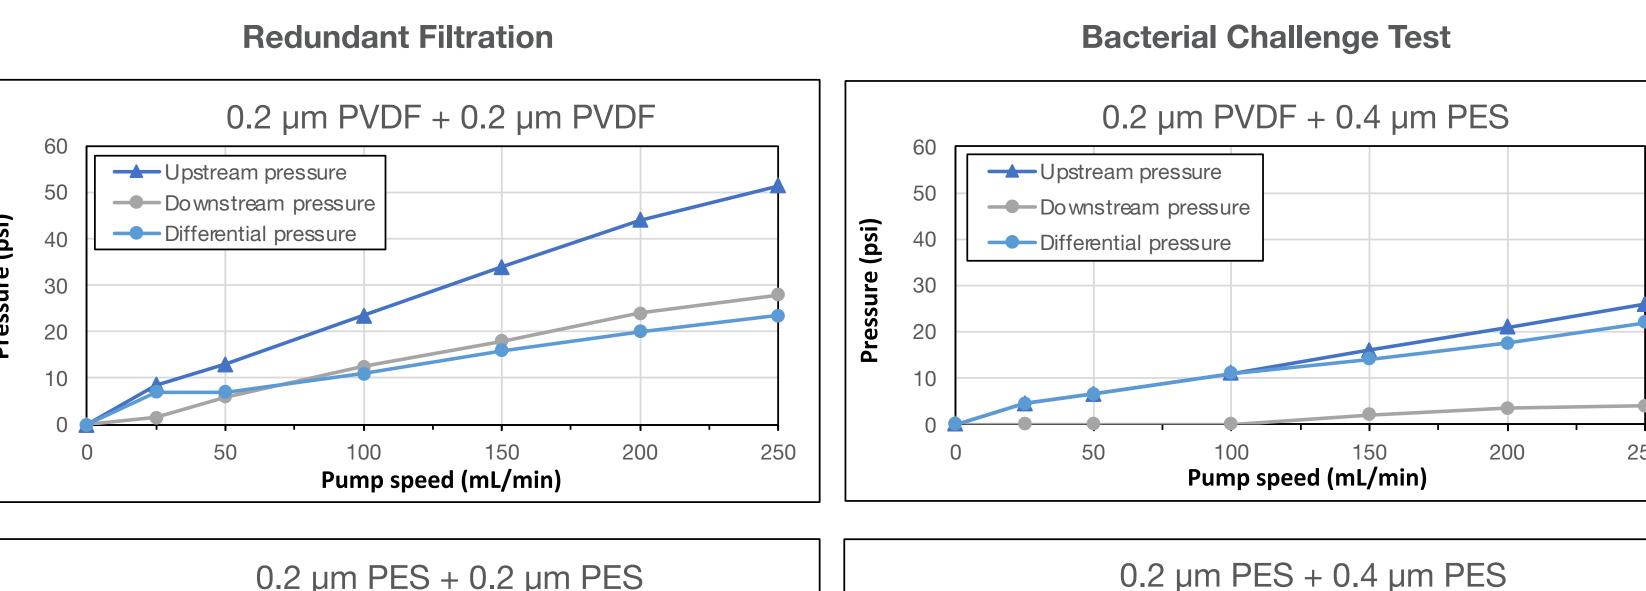

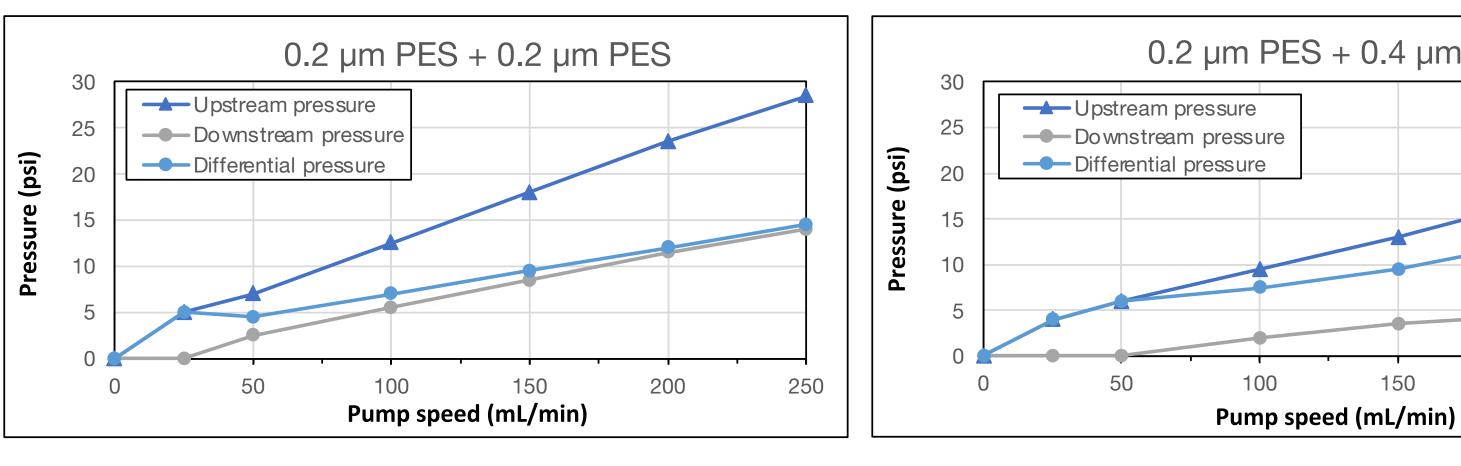


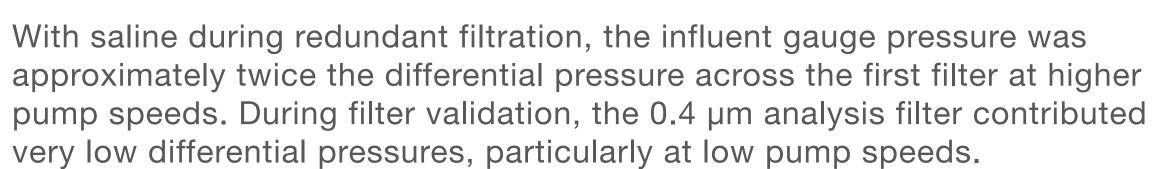

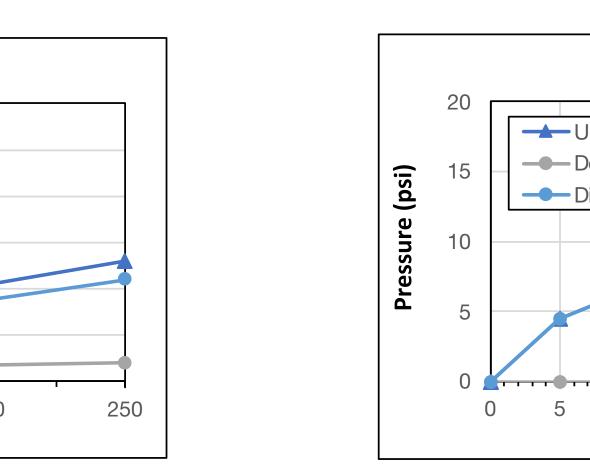

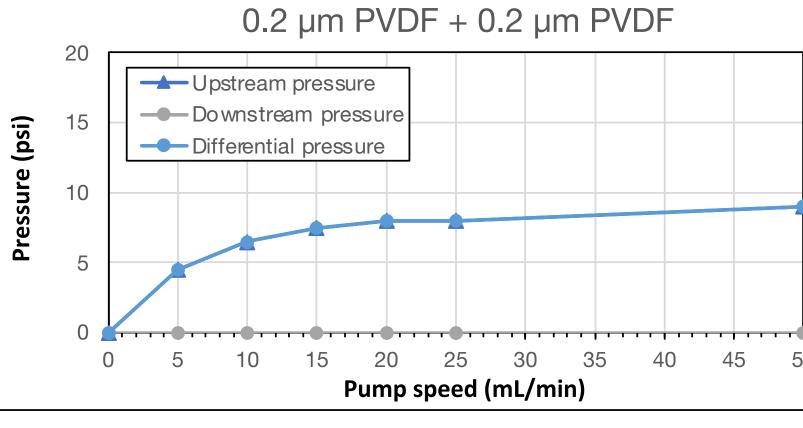

Redundant Filtration

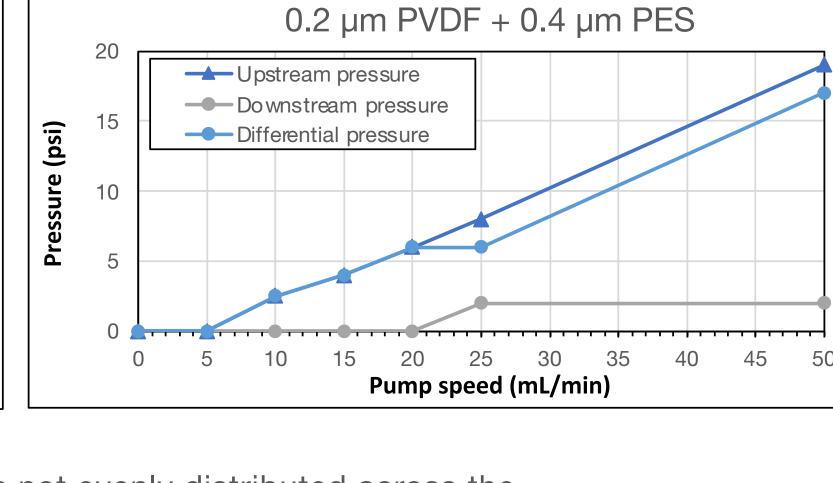



Bacterial Challenge Test


With FBS, the differential pressure was not evenly distributed across the redundant filters. During filter validation, the 0.4 µm analysis filter contributed minimally to the differential pressure on the first filter. The increased pressure on the 0.2 um filter is likely due to the filter plugging, and the low pressure on the analysis filter is due to low flow. Pressure increases as flow decreases when using a constant pump speed.


FBS

DMEM + 10% FBS

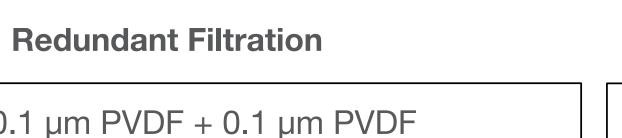


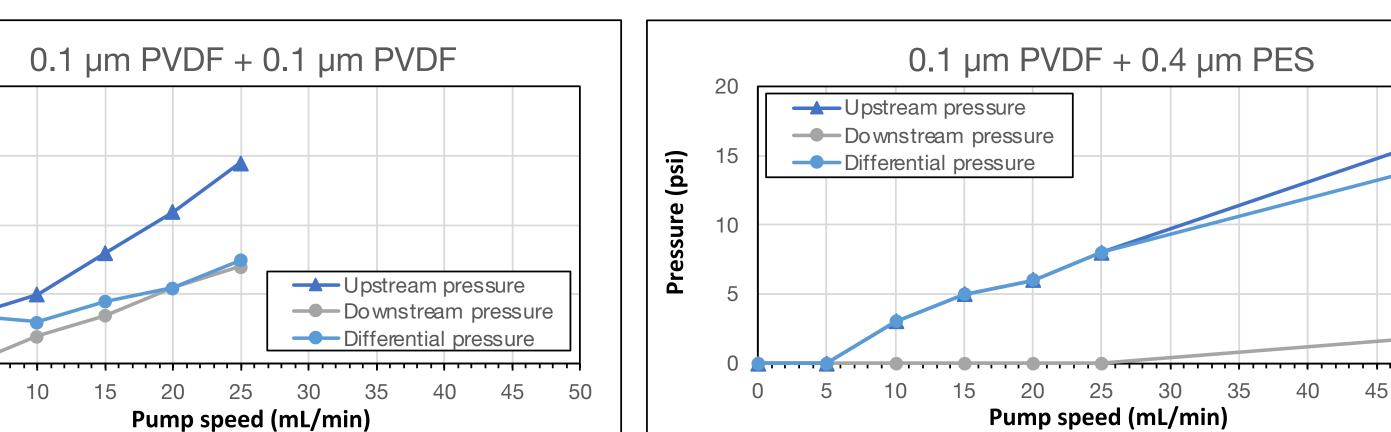

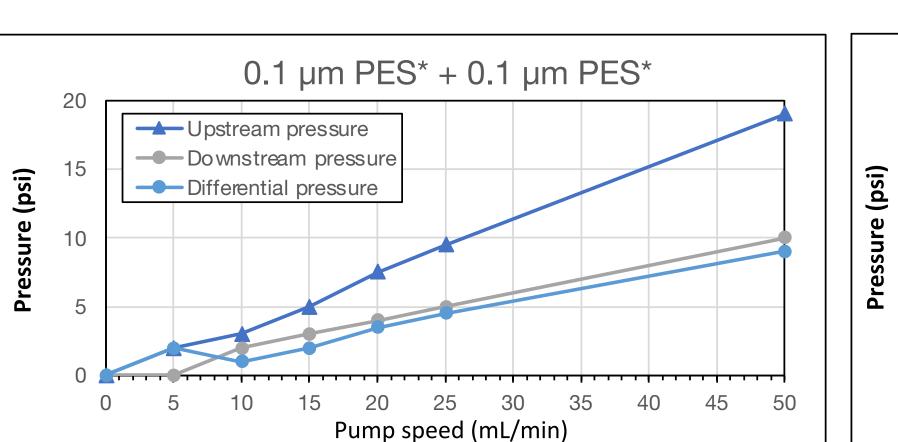

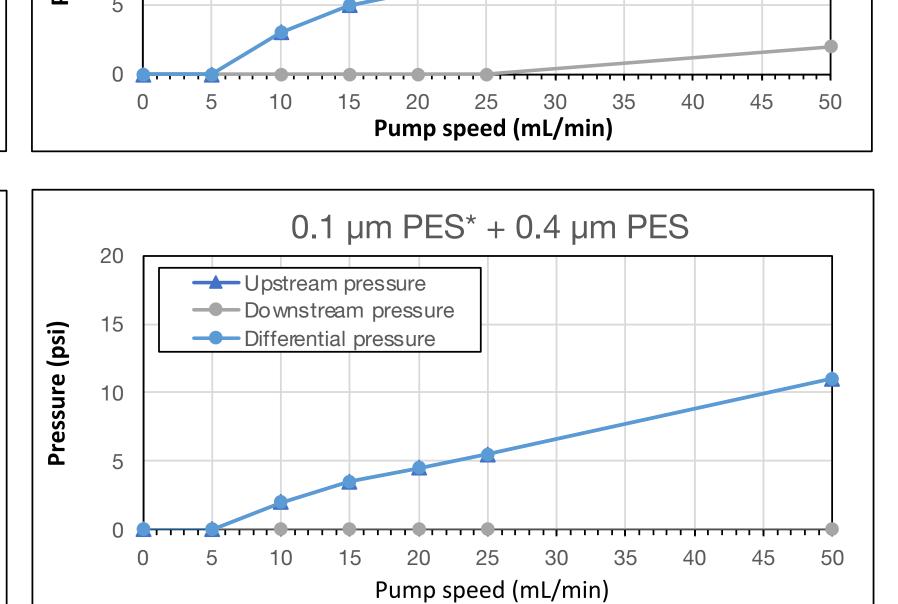



Bacterial Challenge Test

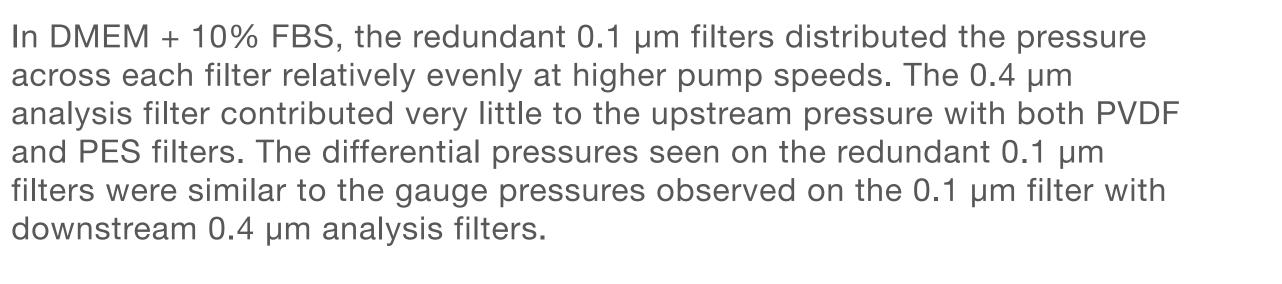



* dual layer 0.1 µm PES

Grapeseed Oil

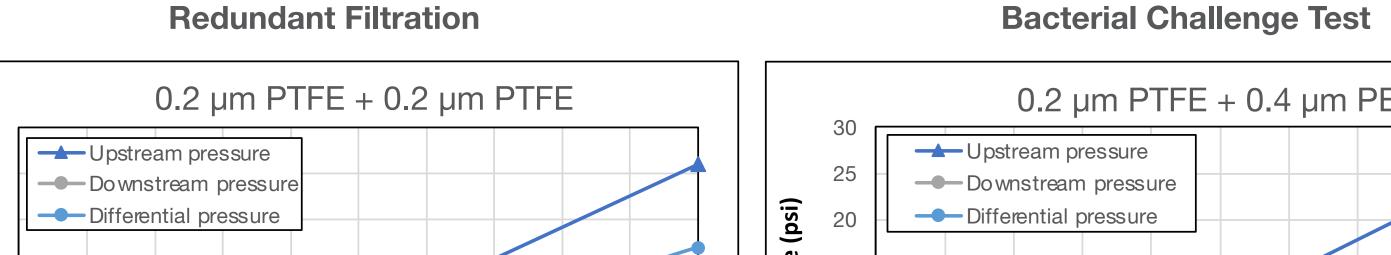

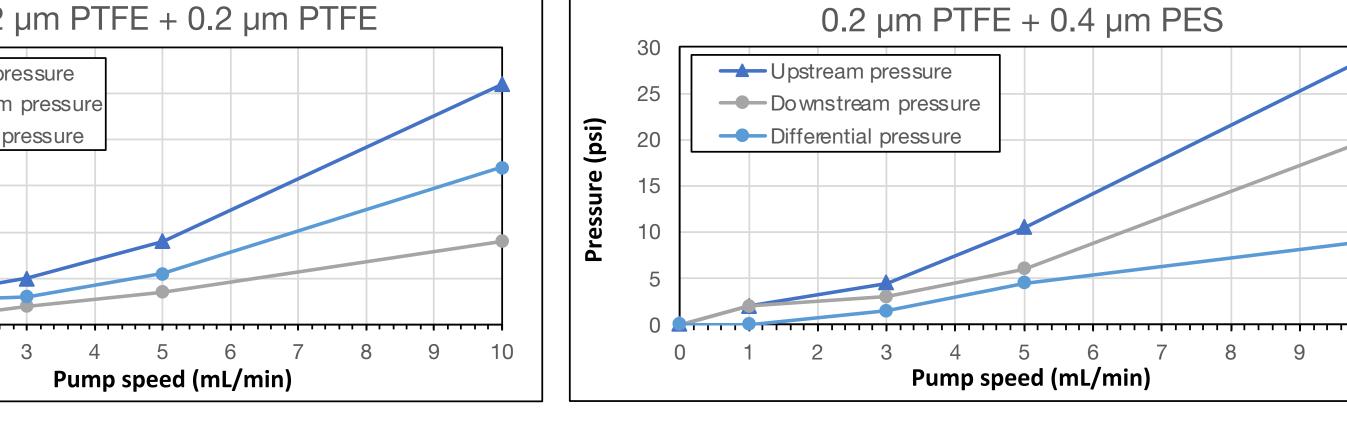

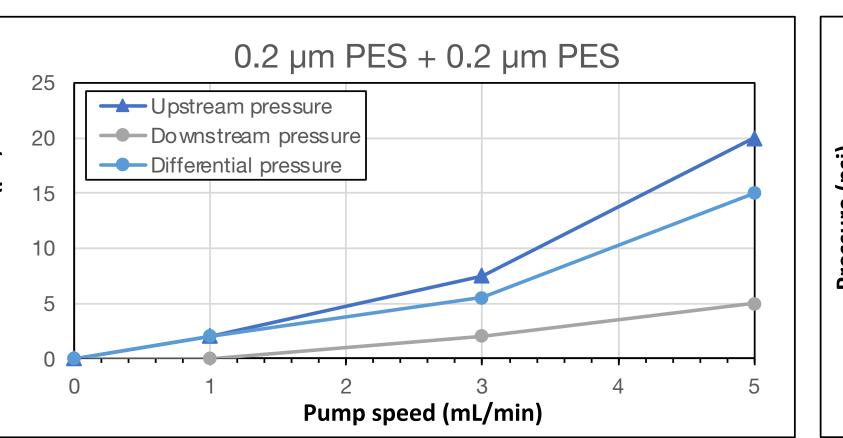

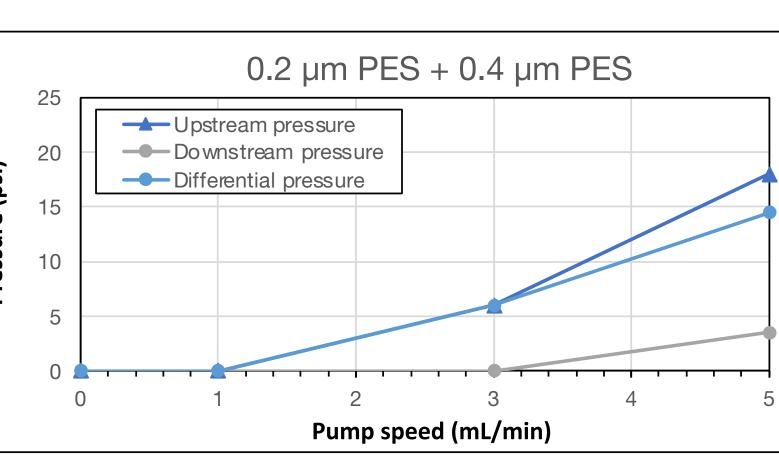

With grapeseed oil, the pressures for the redundant PTFE and PES filters were not evenly distributed; this was more pronounced with the PES filters. The analysis filter contributed significantly to the gauge pressure on the upstream PTFE filter.

Conclusion

In this study, differential pressures across PVDF, PES, and PTFE membrane filters were evaluated during filtration with 0.85% saline, FBS, DMEM + 10% FBS, and grapeseed oil at increasing pump speeds. Our results demonstrate that in non-viscous, aqueous solutions, the feed pressure tends to be distributed evenly across the 2 redundant filters, particularly at high flow rates. Viscous and nonaqueous solutions can behave differently. Bacterial challenge test setups can accurately simulate the actual differential pressures of the redundant filtration processes for aqueous solutions. Furthermore, downstream PES analysis filters made minimal contributions to upstream gauge pressure during filtration with aqueous, low viscosity solutions. Consideration should be given to the selection of analysis membranes during bacterial retention testing.

